



FIG. 1

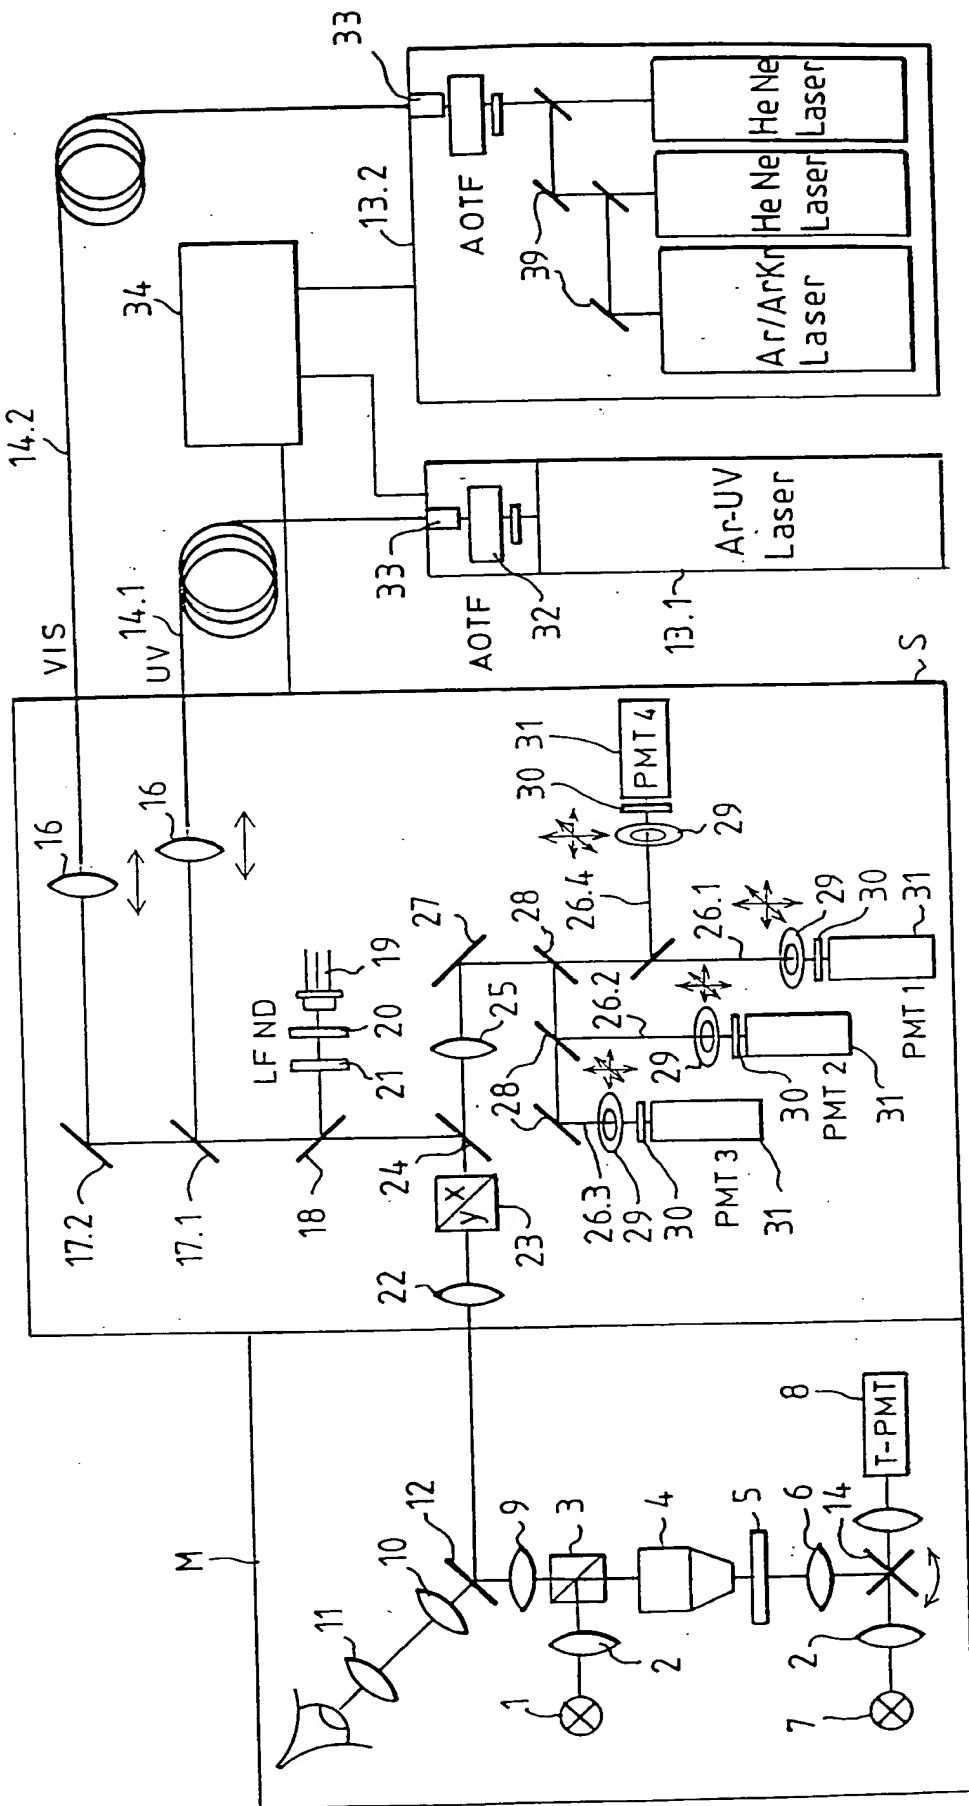

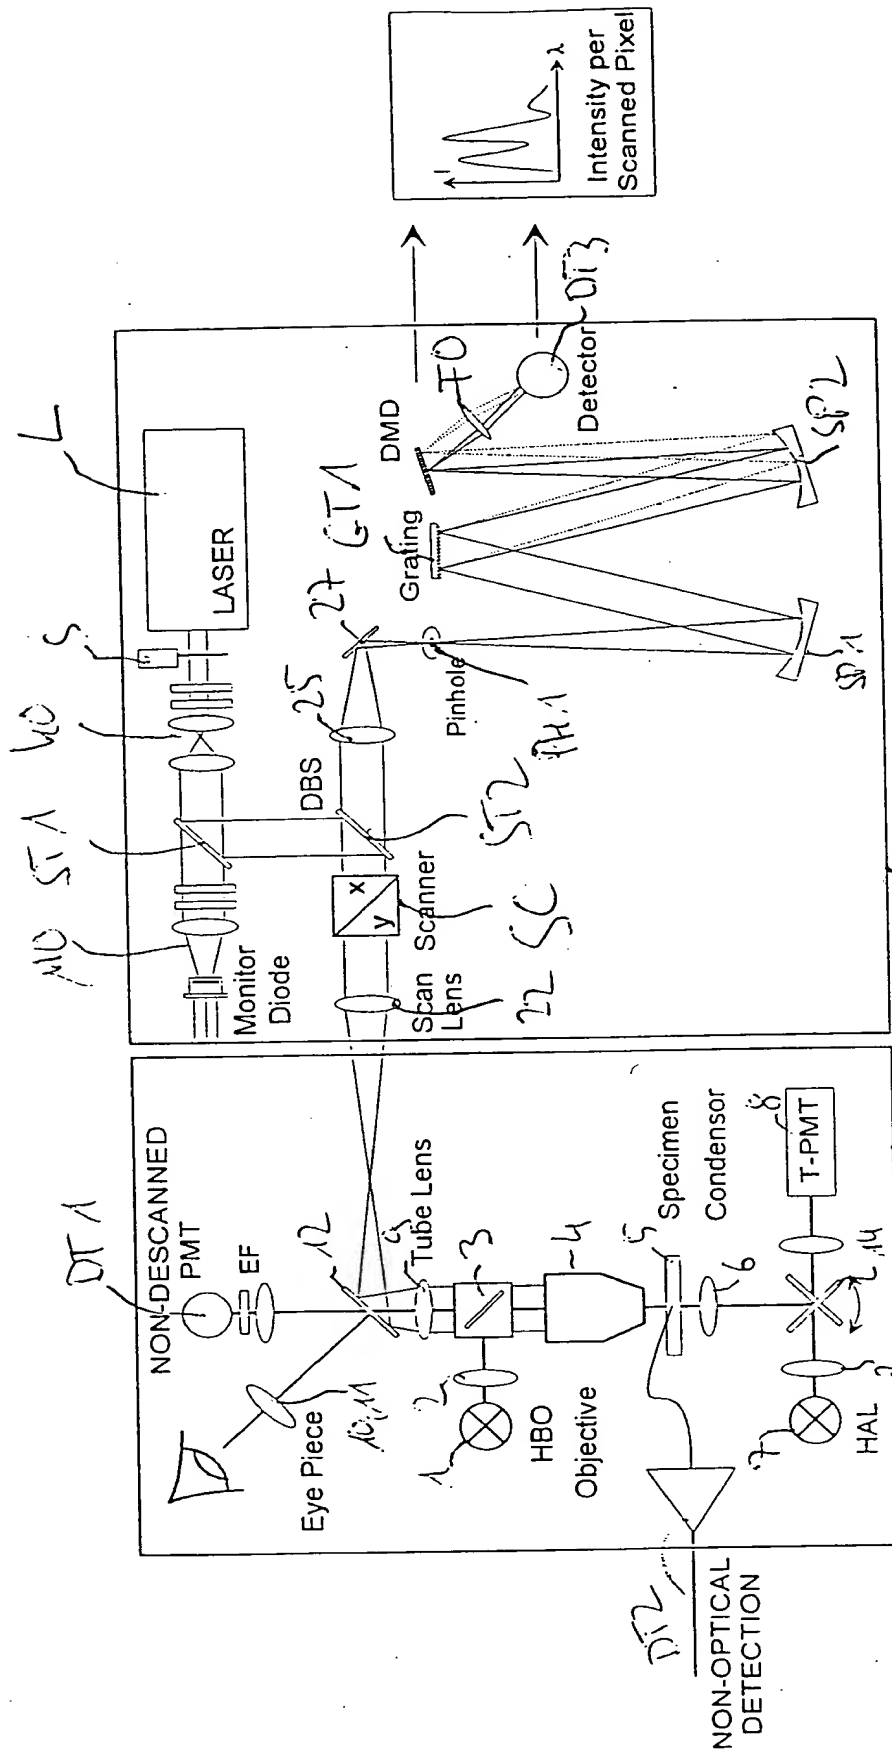

Scan Module

Microscope

FIG. 2

Direction toward
microscope

Fig. 3a

667240" 55556260



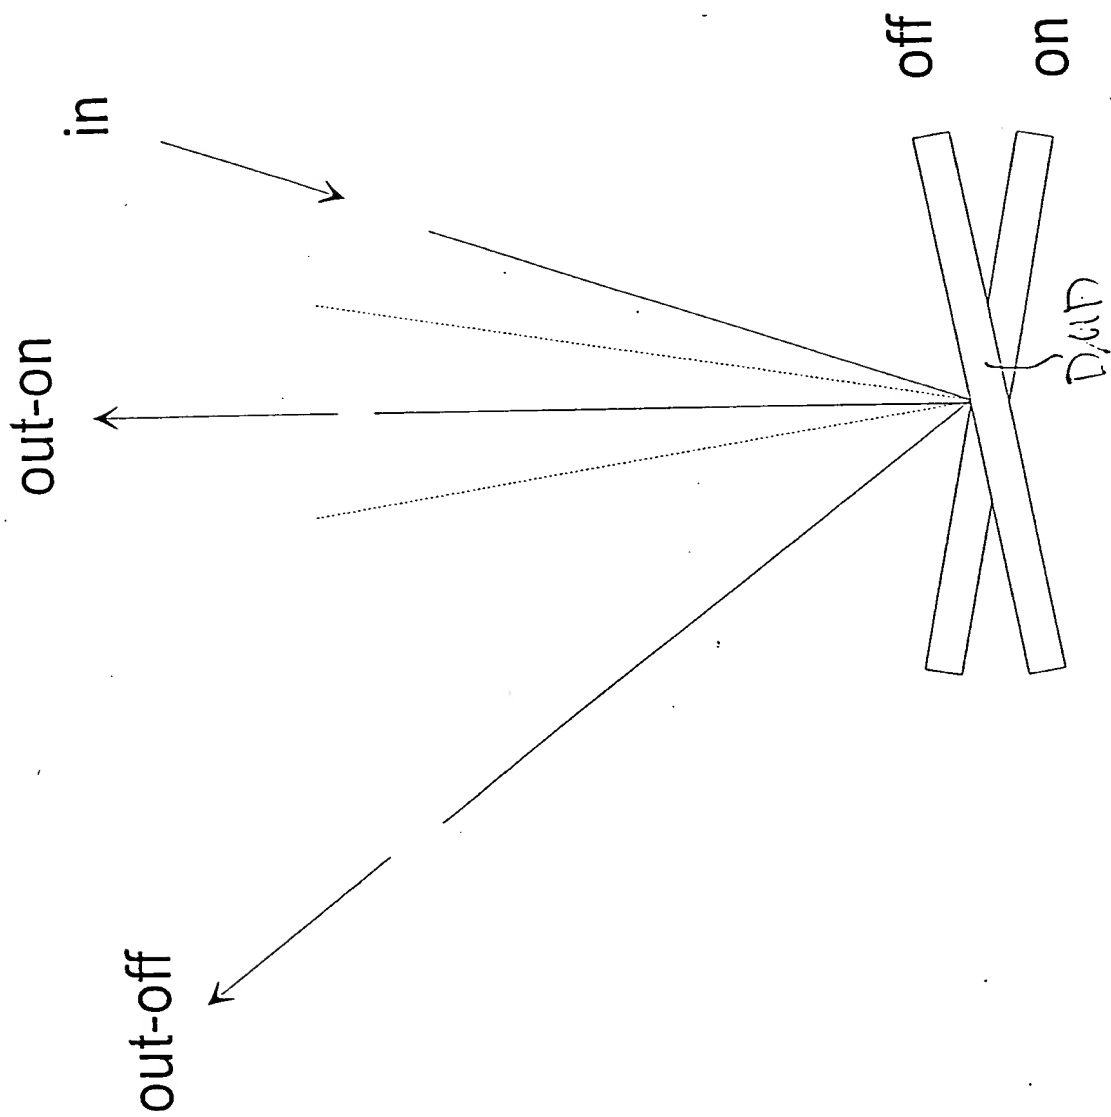


Fig. 3b

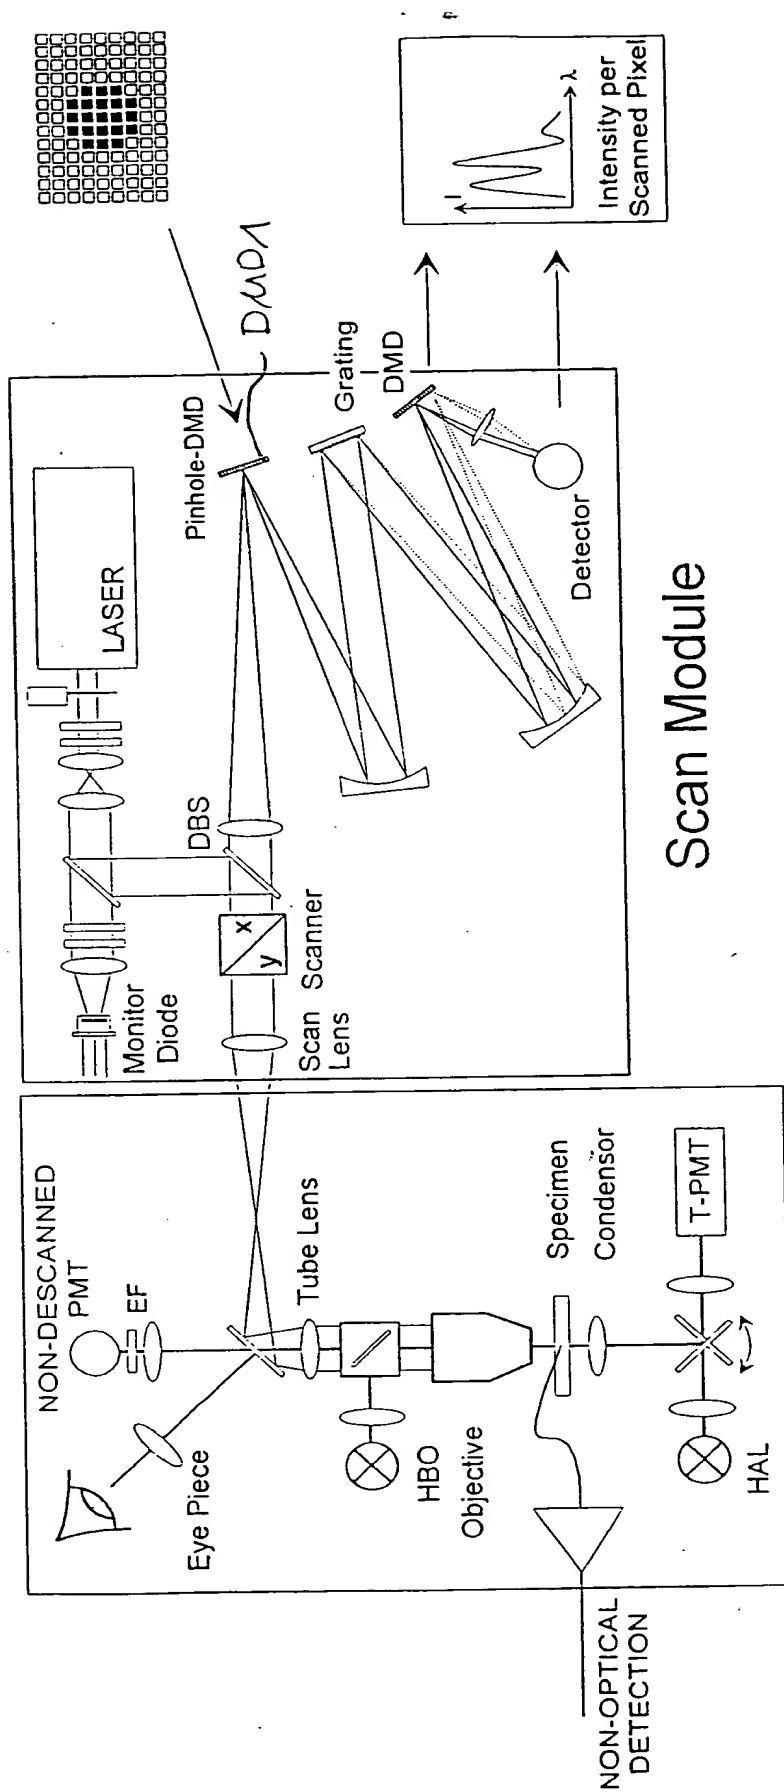


Microscope

Fig. 4.

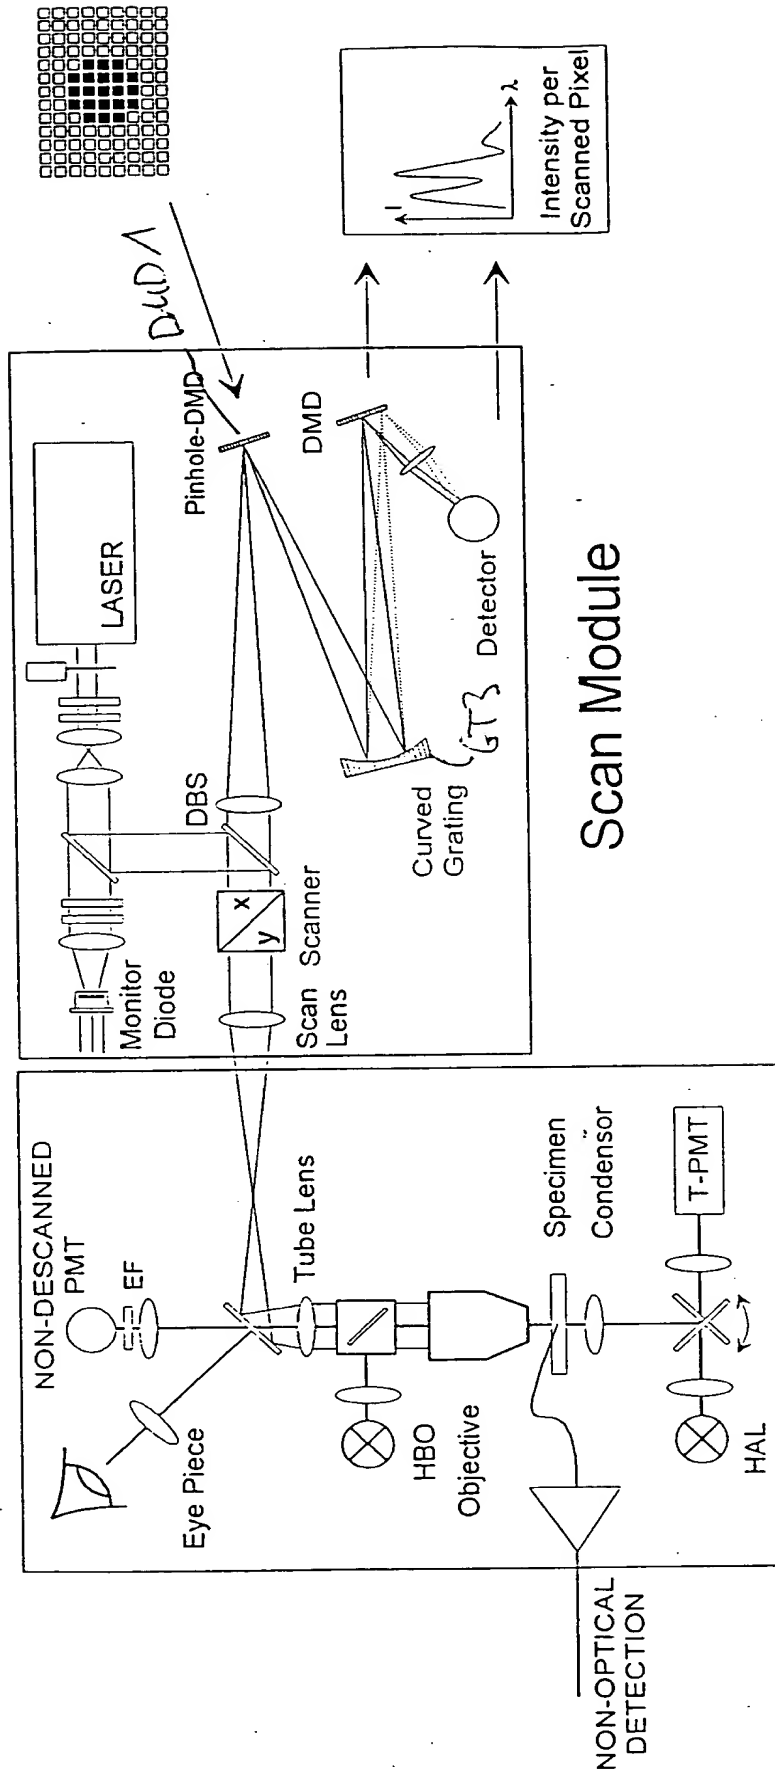

Microscope

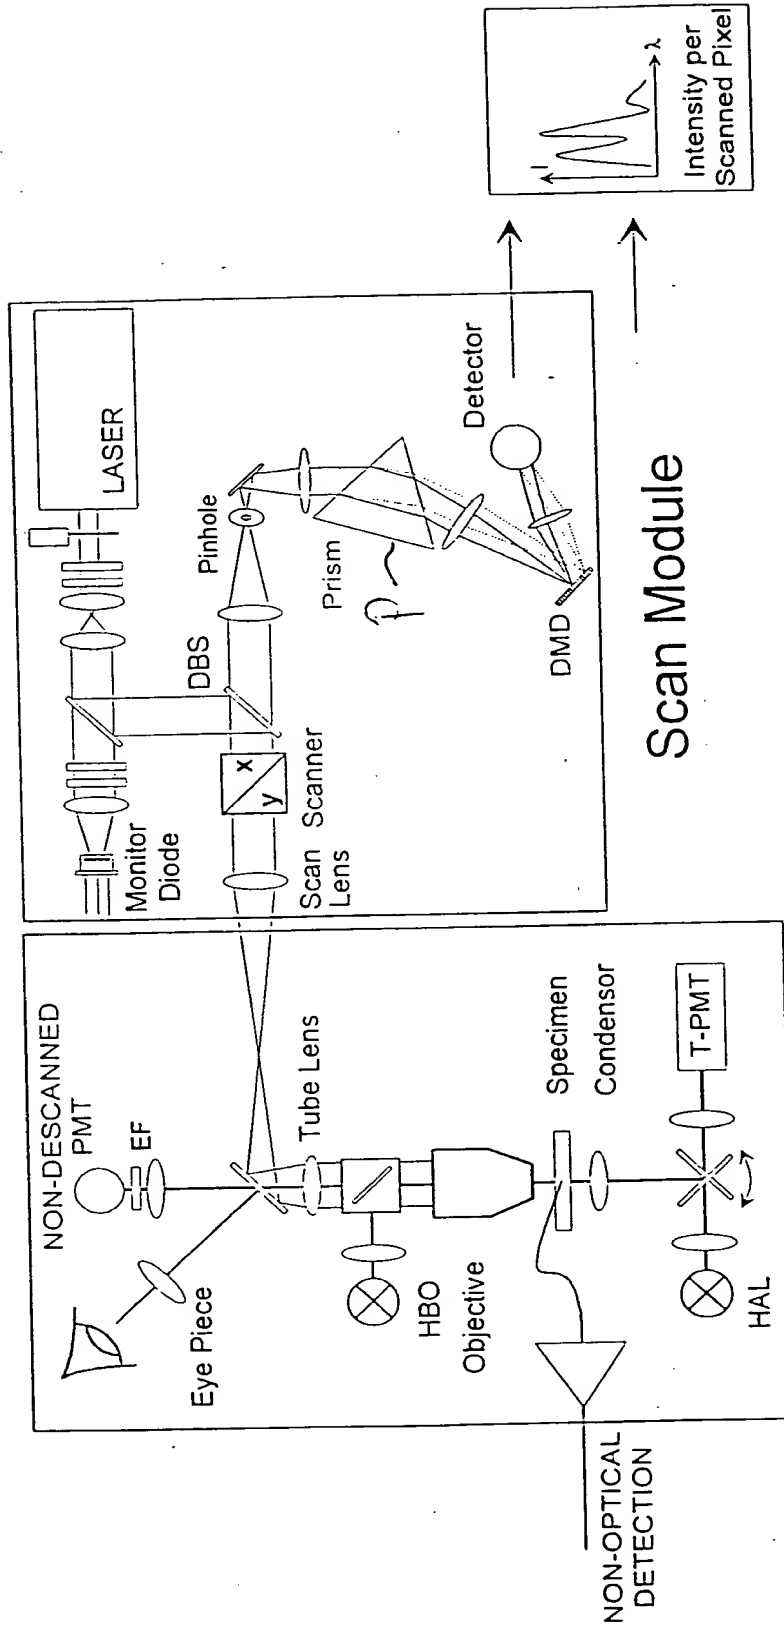

Microscope

Fig. 6.

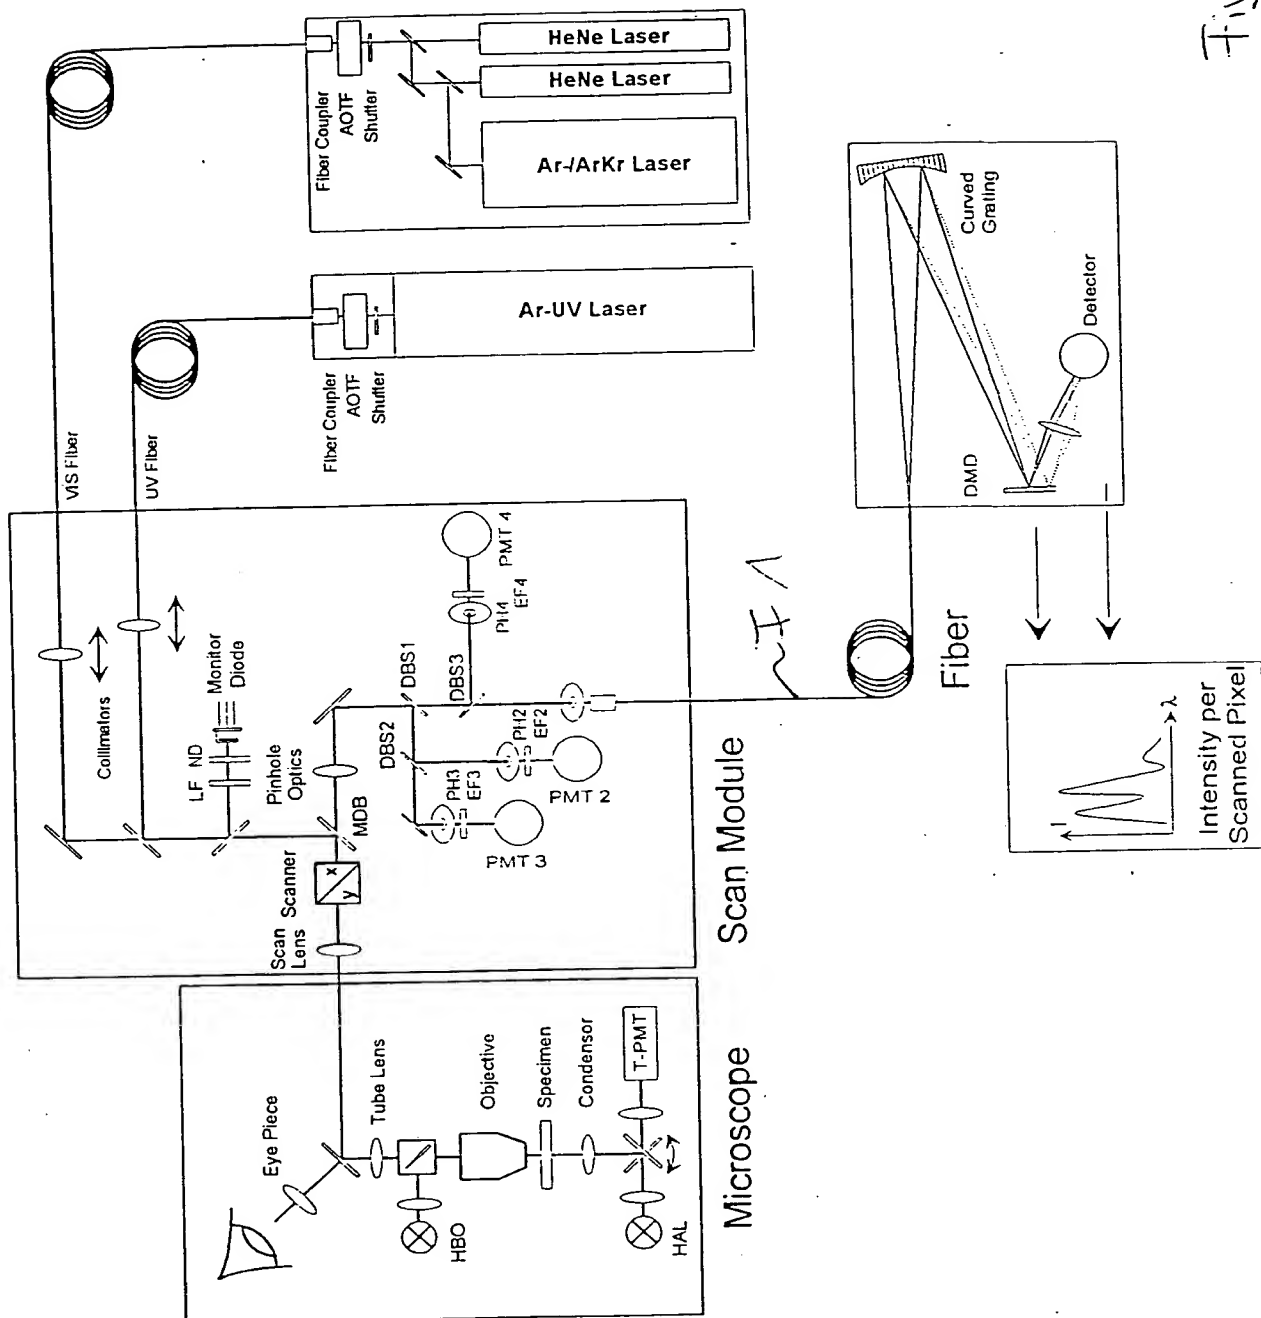


Fig 7.


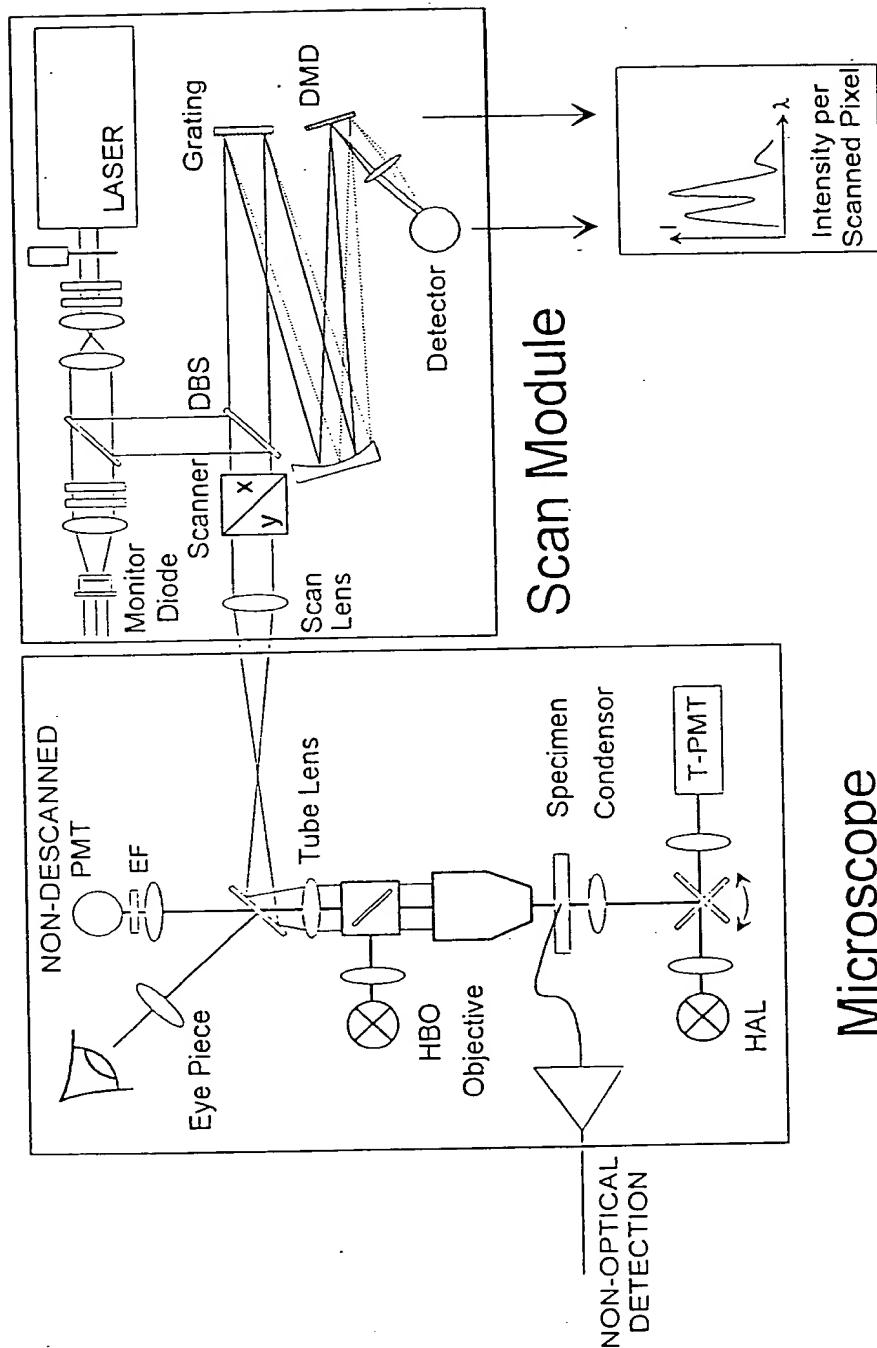


Fig. 2

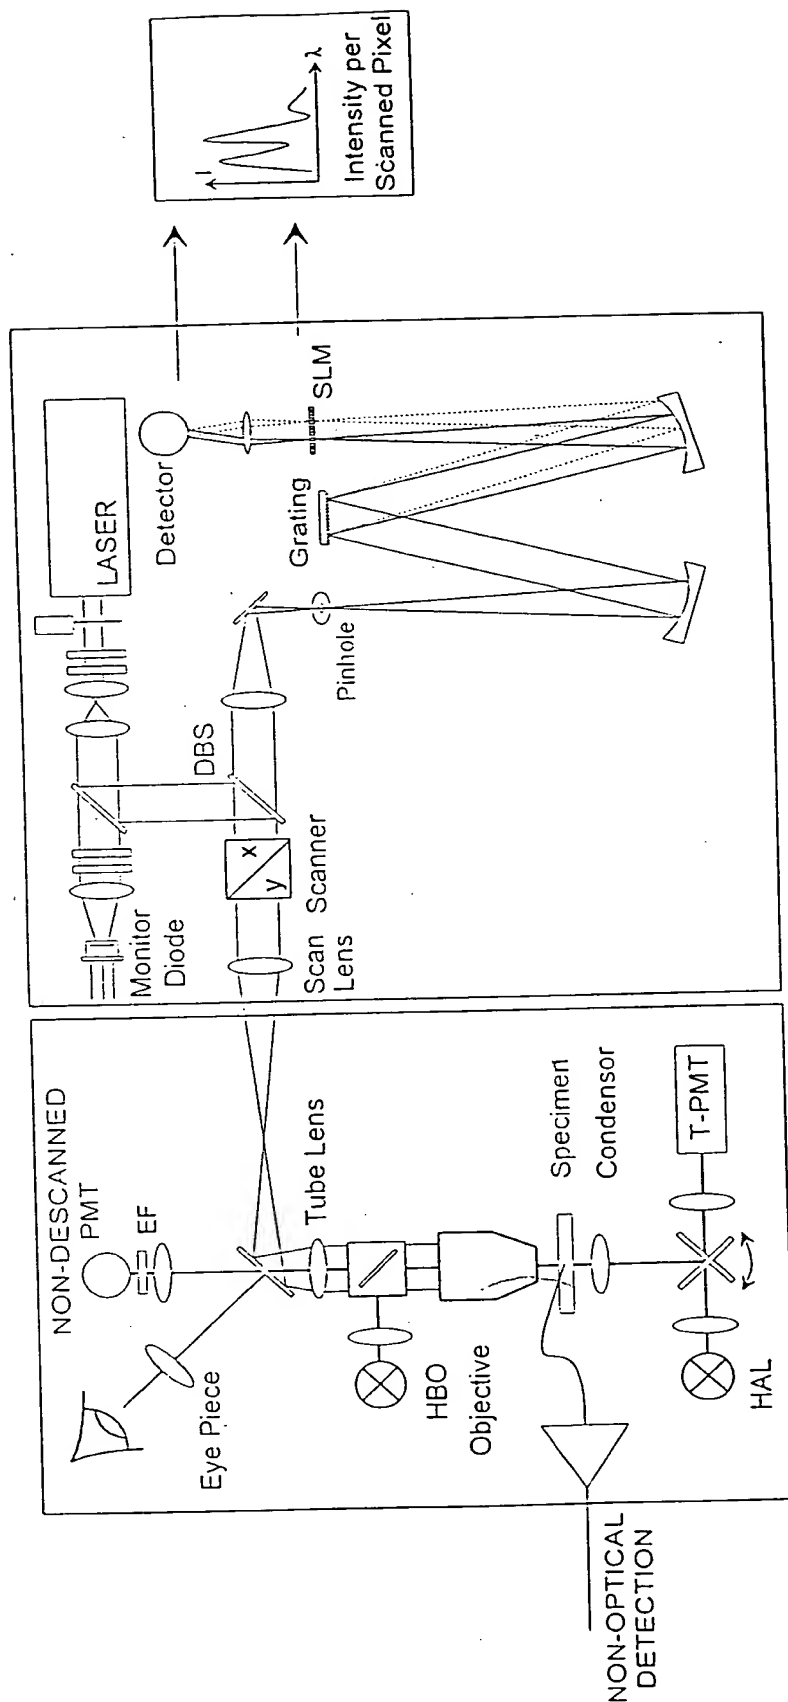

Scan Module

Microscope

F. J. 2

